

OPUS

12SXXXXX0



OPUS is the new generation of spectral sensors for online measurement of nitrogen and carbon compounds. Through the analysis of a full spectrum, OPUS is able to deliver reliable readings for NO₃-N, NO₂-N, organic ingredients (CODeq, BODeq, DOCeQ, TOCeQ), and a number of other parameters.

OPUS features the new TriOS G2 interface, allowing fast and easy configuration of sensors by using a web browser.

Integration into existing process control systems and external data loggers has never been easier.

With the optional battery pack, mobile applications are also feasible. WiFi connectivity allows laptops, tablets or smartphones to be easily used for control without any special application software or app installation.


Benefits

- Without sampling and preparation of test samples
- Real-time sensor
- Without reagents
- Optical window with nano coating
- Pre-installed application calibration

Applications

- Sewage treatment plants
- Environmental monitoring
- Drinking water monitoring
- Industrial applications

Absorption spectrum with/without CODeq

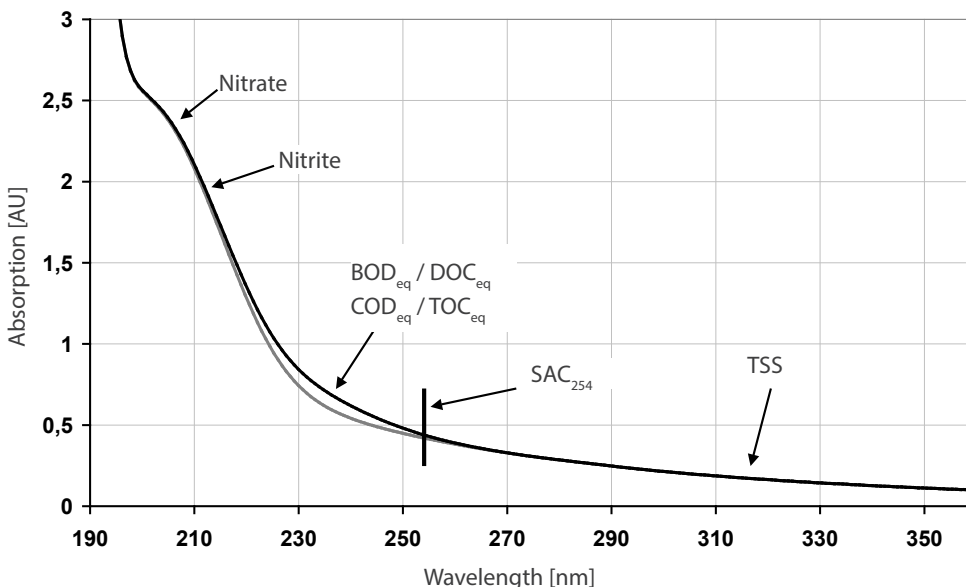

Technical Specifications

Measurement technology	light source	Xenon flash lamp	
	detector	High-end miniature spectrometer	
		256 Channels	
		200 to 360 nm	
		0.8 nm/pixel	
Measurement principle		Attenuation, spectral analysis	
Optical path		0.3 mm, 1 mm, 2 mm, 5 mm, 10 mm, 50 mm	
Parameter		See parameter list p. 3	
Measuring range		See parameter list p. 3	
Measurement accuracy		See parameter list p. 3	
Turbidity compensation		Yes	
Data logger		~ 2 GB	
T100 response time		2 min	
Measurement interval		≥ 1 min	
Housing material		Stainless steel (1.4571/1.4404) or titanium (3.7035)	
Dimensions (L x Ø)		470 mm x 48 mm (with 10 mm path)	~ 18.5" x 1.9" (with 10 mm path)
Weight	stainless steel	~ 3 kg (with 10 mm path)	~ 6.6 lbs (with 10 mm path)
	titanium	~ 2 kg (with 10 mm path)	~ 4.4 lbs (with 10 mm path)
Interface	digital	Ethernet (TCP/IP)	
		RS-232 or RS-485 (Modbus RTU)	
Power consumption		≤ 8 W	
Power supply		12...24 VDC (± 10 %)	
Maintenance effort		≤ 0.5 h/month (typical)	
Calibration/maintenance interval		24 months	
System compatibility		Modbus RTU	
Warranty		1 year (EU: 2 years)	US: 2 years
INSTALLATION			
Max. pressure	with SubConn	30 bar	~ 435 psig
	with fixed cable	3 bar	~ 43.5 psig
	in FlowCell	1 bar, 2...4 L/min	~ 14.5 psig at 0.5 to 1.0 gpm
Protection type		IP68	NEMA 6P
Sample temperature		+2...+40 °C	~ +36 °F to +104 °F
Ambient temperature		+2...+40 °C	~ +36 °F to +104 °F
Storage temperature		-20...+80 °C	~ -4 °F to +176 °F
Inflow velocity		0.1...10 m/s	~ 0.33 fps to 33 fps

Measuring Range

Single parameter under optimum laboratory conditions

Path (mm)	Parameter	Measurement principle	Unit	Measuring range	Detection limit	Limit of determination	Precision	Accuracy*
1	Nitrate NO ₃ -N	Spectral	mg/L	0...100	0.3	0.5	0.05	± (5 % + 0.1)
	Nitrite NO ₂ -N	Spectral	mg/L	0...150	0.5	1.2	0.12	± (5 % + 0.1)
	CODeq	Spectral	mg/L	0...2200***	30	100	10	
	BODeq	Spectral	mg/L	0...2200***	30	100	10	
	DOCe _q	Spectral	mg/L	0...1000	5	10	1	
	TOCe _q	Spectral	mg/L	0...1000	5	10	1	
	TSSe _q	Spectral	mg/L	0...1500	60	200	20	
	KHP	Spectral	mg/L	0...4000	5	10	1	± (5 % + 2)
	SAC ₂₅₄	Single wavelength	1/m	0...2200	15	50	5	
	COD-SACe _q **	Single wavelength	mg/L	0...3200	22	73	7.3	
BOD-SACe _q **	Single wavelength	mg/L	0...1050	7.2	24	2.4		
10	Nitrate NO ₃ -N	Spectral	mg/L	0...10	0.03	0.05	0.005	± (5 % + 0.01)
	Nitrite NO ₂ -N	Spectral	mg/L	0...15	0.05	0.12	0.012	± (5 % + 0.01)
	CODeq	Spectral	mg/L	0...220***	3	10	1	
	BODeq	Spectral	mg/L	0...220***	3	10	1	
	DOCe _q	Spectral	mg/L	0...100	0.5	1	0.1	
	TOCe _q	Spectral	mg/L	0...100	0.5	1	0.1	
	TSSe _q	Spectral	mg/L	0...150	6	20	2	
	KHP	Spectral	mg/L	0...400	0.5	1	0.1	± (5 % + 0.2)
	SAC ₂₅₄	Single wavelength	1/m	0...220	1.5	5	0.5	
	COD-SACe _q **	Single wavelength	mg/L	0...320	2.2	7.3	0.73	
BOD-SACe _q **	Single wavelength	mg/L	0...105	0.72	2.4	0.24		

* Based on a standard calibration solution

** Based on KHP (100 mg/L COD standard solution correspond to 85 mg/L KHP)

*** Depending on composition of COD and BOD (checksum parameter)

1 mg/L NO₃-N correspond to 4.43 mg/L NO₃

1 mg/L NO₂-N correspond to 3.28 mg/L NO₂



OPUS G2 Interface

The easiest and fastest way of sensor integration and configuration in any process control system or data logger via web browser:

Let OPUS automatically monitor your processes and react to unexpected events or incidents with the optional "policing" feature of OPUS.



**We represent this supplier.
For more information contact
Observator Instruments:**

**T: +31 (0)180 463411
E: info@observator.com**

Rietdekkerstraat 6
2984 BM Ridderkerk
The Netherlands

Welcome to the world of Observator

Since 1924 Observator has evolved to be a trend-setting developer and supplier in a wide variety of industries. Originating from the Netherlands, Observator has grown into an internationally

oriented company with a worldwide distribution network and offices in Australia, Germany, the Netherlands, Singapore and the United Kingdom.

www.observator.com